

Date: 2023.01.22; update: 2023.02.13; update: 2023.02.23

Field Safety Notice
Belzer UW[®] Cold Storage Solution; Belzer MPS[®]
& StoreProtect[®]

For Attention of*: Distributors, Importers, Hospitals, Health Care Professionals

Contact details of local representative (name, e-mail, telephone, address etc.)*

Legal Manufacturer:

Carnamedica Sp. z o.o.
21/U6 Olszynki Grochowskiej St.
04-281 Warsaw
Poland
e-mail: vigilance@carnamedica.com

Distributors of Belzer UW[®] Cold Storage Solution, Belzer MPS[®]:

Bridge to Life Europe Ltd.
LU 311 The Light Bulb
1 Filament Walk
London SW18 4GQ
Phone: +44(0)20 3411 8326
Fax: +44 (0)20 3004 1103
<https://bridgetolife.eu/contact-bridge-to-life-ltd/>

Bridge to Life Ltd.
Logistics & Ordering: 128 Suber Rd. Suite A
Columbia, SC 29210; USA

Distributor of StoreProtect[®], Belzer MPS[®] (Poland):

Infusion
21/U6 Olszynki Grochowskiej St.
04-281 Warsaw
Poland
e-mail: vigilance@carnamedica.com

Field Safety Notice (FSN)
Belzer UW[®] Cold Storage Solution; Belzer MPS[®]
& StoreProtect[®]

1. Information on Affected Devices*	
1.	<p>1. Device Type(s)*</p> <ul style="list-style-type: none"> • Belzer UW[®] Cold Storage Solution (University of Wisconsin Solution) <i>Container with perfusion and preservation solution for organs intended for transplantation</i> • Belzer MPS[®] (UW Machine Perfusion Solution) <i>Container with perfusion and preservation solution for organs intended for transplantation</i> • StoreProtect[®] <i>Container with perfusion and preservation solution for organs intended for transplantation</i>
1.	<p>2. Commercial name(s)*</p> <ul style="list-style-type: none"> • Belzer UW[®] • Belzer MPS[®] • StoreProtect[®]
1.	<p>3. Unique Device Identifier(s) (UDI-DI)</p> <p>See Appendix A to this FSN.</p>
1.	<p>4. Primary clinical purpose of device(s)*</p> <ul style="list-style-type: none"> • Belzer UW[®] Belzer UW[®] Cold Storage Solution (University of Wisconsin Solution) is a clear to light yellow, sterile, non-pyrogenic solution intended for the flushing and the hypothermic storage of organs (kidney, liver, pancreas) or other organs at the time of organ removal from the donor, in preparation for storage, transportation and eventual transplantation into the recipient. • Belzer MPS[®] Belzer MPS[®] (UW Machine Perfusion Solution) perfusion solution is a clear to slightly yellow, sterile, non-pyrogenic, non-toxic solution for the in-vitro flushing and temporary continuous hypothermic machine perfusion of organs during their storage, transportation, until transplantation into a recipient. • StoreProtect[®] StoreProtect[®] is a clear to light yellow, sterile, non-pyrogenic solution intended for the flushing and the hypothermic storage of organs (kidney, liver, pancreas) or other organs at the time of organ removal from the donor, in preparation for storage, transportation and eventual transplantation into the recipient.
1.	<p>5. Device Model/Catalogue/part number(s)*</p> <p>See Appendix A to this FSN.</p>
1.	<p>6. Software version</p> <p>Not applicable</p>
1.	<p>7. Affected serial or lot number range</p> <p>See Appendix A to this FSN.</p>
1.	<p>8. Associated devices</p> <p>Not applicable</p>

2. Reason for Field Safety Corrective Action (FSCA)*	
2.	<p style="text-align: center;">1. Description of the product problem*</p> <p>Carnamedica Sp. z o.o., with this Field Safety Notice is initiating a voluntary suspension to supply for the sterile Belzer UW®, Belzer MPS® and StoreProtect® (the list of reference codes and LOT numbers is included in the Appendix A), effective immediately.</p> <p>Carnamedica has determined the following issues related to these devices:</p> <ul style="list-style-type: none"> ▪ leaking within the solution bag overwrap, ▪ turbidity and discoloration; ▪ visible particulates. <p>The defects are immediately identifiable upon product acceptance prior to the use of the solution. The affected devices were shipped during the time frame of 12.2021 – 11.2022.</p>
2.	<p style="text-align: center;">2. Hazard giving rise to the FSCA*</p> <p>A damaged or leaking bag could result in microbial contamination of the sterile solution path due to lose of the sterile barrier. The turbidity and obvious intense discoloration is an indication of microbial contamination. This may predispose patients to peritonitis, infection, sepsis and failure to graft. Additional potential hazards that may result include delay in therapy.</p> <p>If the visible particles are isolated in the device, local post-reperfusion ischemia may occur and there may be a potential risk of delayed graft function due to obliteration of some small vessels.</p> <p>The risk is mitigated by the end user during the organs' preparation procedure according to the Instructions for Use (IFU), section PREPARATION. It is an obligatory standard for the end user to check each container that is used for presence of leakage/ discoloration or foreign particles, before the solution is administrated into the organ. In case that the solution contains any visible particles/ discoloration/ leakage, the product must be discarded and cannot be used for the patient.</p>
2.	<p style="text-align: center;">3. Probability of problem arising</p> <p>There have been no serious injuries associated with leakage/ discoloration or particles that were reported in the accessible literature.</p> <p>There are a handful of reports that cite near-miss situations, without actual injury, and the majority are discussing theoretical adverse events based on common medical knowledge but without real life proof of occurrence. It implies that the probability that the devices create hazardous situation leading to an injury is very low/ unlikely. The devices are used by the Health Care Professional user.</p>
2.	<p style="text-align: center;">4. Predicted risk to patient/users</p> <p>Based on the internal and external investigations, the Medical Assessment part of the Health Hazard Evaluation (HHE) where the risk involved is theoretical and given that no identifiable studies relating to leakage/ discoloration or particles incidents leading to an adverse event are evident, and the lack any reports to Carnamedica of injury related to that.</p> <p>The risk is mitigated by the end user during the organs' preparation procedure and should not to cause adverse health consequences. All risks were identified by the manufacturer within the risk analysis and the information about such remaining risks is incorporated into the Instruction for Use (IFU).</p>
2.	<p style="text-align: center;">5. Further information to help characterise the problem</p> <p>Leakages and turbidity/ discoloration occur when the sterile barrier of the product is lost. Several factors can cause these defects: the EVA bag micro-sealing issue, the EVA bag injection port issue, the aseptic process issue. These issues affect only the individual affected bags, not the entire batch (LOT). The original issue is related to the individual EVA bags and can contribute to the aseptic process and result in microbiological contamination.</p> <p>The presence of visible particles in the solution is the result of overheating caused by failure to meet the manufacturer's specified transport/ storage temperature in the supply chain.</p>

	This issue is limited to Belzer UW® and Belzer MPS® solutions caused by improper product's handling and distribution.
2.	6. Background on Issue Customers reported an increase number of defects related to the leakages, discoloration and particles in the solutions before the use. None of the complaints report any patient adverse events.
2.	7. Other information relevant to FSCA Stop any further use of the affected devices.

3. Type of Action to mitigate the risk*

3. 1. Action To Be Taken by the User*

- Identify Device
 Quarantine Device
 Return Device
 Destroy Device

 On-site device modification / inspection

 Follow patient management recommendations

 Take note of amendment / reinforcement of Instructions For Use (IFU)


 Other None


We would appreciate your assistance in the following actions:

1. **Read** the "2.1. Description of the product problem" section carefully to fully understand the issue involved.
2. Please immediately **examine** your inventory stock to determine if you have any remaining product in your possession.
3. **Stop** any further sale and distribution/ usage of the affected product.
4. The following illustrations are provided to help you identify the products and lots. Affected lots are identified by the reference number and lot number on the bag and case labels.

Bag labels








1 Container filled with organ perfusion and preservation solution
 Recipiente con la solución para perfusión y preservación de órganos
 Conteneur avec solution pour perfusion et conservation des organes
 Behälter mit Lösung zur Durchblutung und Konservierung der Organe
 Behälter med perfusionsvätska och vätskor för transplanterade organ
 Recipiente com a solução para preservação de órgãos
 Контейнер для перфузии и хранения органов, предназначенный для трансплантации

Warning: Not intended for systemic administration by direct injection or intravenous infusion.	Warning: Not for in situ flushing of organs in living donors or patients.	Warning: Discard any unused portion.
Advertencia: No está destinado a la administración sistémica mediante inyección directa o por perfusión intravenosa.	Advertencia: No apto para la irrigación de órganos in situ en donantes o pacientes vivos.	Advertencia: Discarte cualquier porción no utilizada.
Avertissement: Non destiné à une administration par voie générale et injection directe ou perfusion intraveineuse.	Avertissement: Non destiné au rinçage in situ d'organes sur les donneurs vivants ou les patients.	Avertissement: Jeter toute portion inutilisée.
Attenzione: Non destinato alla somministrazione sistemica mediante iniezione diretta o infusione endovenosa.	Attenzione: Non idoneo per il lavaggio in situ di organi in donatori o pazienti viventi.	Attenzione: Scartare eventuali residui.
Warnhinweis: Nicht zur systemischen Verabreichung durch Direktinjektion oder intravenöse Infusion bestimmt.	Warnhinweis: Nicht zur in-situ-Spülung von Organen im Körper lebender Spender oder Patienten.	Warnhinweis: Nicht verbrauchte Teil entsorgen.
Observed: produkten är inte avsedd för injektion och direkt infusering.	Observed: använd ej produkten för att jäja organ hos levande donatorer eller patienter.	Observed: övriga delen av produkten ska slivas ut.
Aviso: Não se destina a administração sistémica por injeção directa ou infusão intravenosa.	Aviso: Não se destina à irrigação in situ de órgãos em doadores vivos ou doentes.	Aviso: Rejeitar qualquer porção não utilizada.
Внимание: не предназначен для инъекций и прямой инфузии.	Внимание: не использовать для промывки органов живых доноров и пациентов.	Внимание: отбраковать часть продукции, которую нельзя использовать.

The reference number is located here


REF BMPSC

LOT XXXXXX



The lot number is located here


Case label



The lot number is located here

REF BMPSC

LOT 111111



The reference number is located here

Actions related to the distributors/ importers:

1. **Conduct** a physical count and **record** the data on the Distributor/Importer Reply Form (in case of the distributors/ importers) attached to this Notice.
2. **Place** reviewed product into quarantine and **return** to the manufacturer.
3. **Return** the Distributor/Importer Reply Form to:
 - your local representative/ distributor (in country BTL representative: f.harvey@b2ll.com and m.harper@b2ll.com);
 - or via e-mail to vigilance@carnamedica.com.

This is important to complete even, if you have no affected product on hand. Please ensure the form contains a contact name and signature.
4. **Contact** your local representative/ distributor (in country BTL representative or <https://bridgetolife.eu/contact-bridge-to-life-ltd/>) or Carnamedica's Service on office@carnamedica.com to understand how to obtain a credit note against affected product and organize the product's return.
5. **Maintain** awareness of this Notice until all affected product has been inspected/ destroyed.
6. **Share** this Notice with anyone who needs to be informed in your facility, or in any facility where potentially affected devices may have been transferred.
7. For any questions about the recall process, please **contact** your local representative/ distributor (in country BTL representative Mr. Mark Harper – Bridge to Life QA Director – m.harper@B2LL.com) or Carnamedica at vigilance@carnamedica.com.

Actions related to the Health Care Professionals:

1. **Conduct** a physical count and **record** the data on the Customer Reply Form (in case of the hospitals/ clinics/ etc.) attached to this Notice.
2. **Perform** and additional visual inspections according to the **Appendix B** to identify bags of solution that may represent leaking, discoloration, and contamination with particles prior to use of product. Before any use of the product, check their condition according to the IFU (Instructions for Use), section **PREPARATION**.
3. **Dispose** of the affected products through waste system, recycle packaging and **document** that on the Customer Reply Form attached to this Notice. If there is no possibility to dispose of the product in this way, you may return the product to local Customer representative through your normal means.
4. **Return** the Customer Reply Form to:
 - your local representative/ distributor (in country BTL representative: f.harvey@b2ll.com and m.harper@b2ll.com);
 - or via e-mail to vigilance@carnamedica.com.

This is important to complete even, if you have no affected product on hand. Please ensure the form contains a contact name and signature.
5. **Contact** your local representative/ distributor (in country BTL representative or <https://bridgetolife.eu/contact-bridge-to-life-ltd/>) or Carnamedica's Customer Service on office@carnamedica.com to understand how to obtain a credit note against affected product.
6. **Maintain** awareness of this Notice until all affected product has been inspected/ destroyed.
7. **Share** this Notice with anyone who needs to be informed in your facility, or in any facility where potentially affected devices may have been transferred.
8. For any questions about this process, please **contact** your local representative/ distributor (in country BTL representative Mr. Mark Harper – Bridge to Life QA Director – m.harper@B2LL.com) or Carnamedica at vigilance@carnamedica.com.

2. By when should the action be completed?

The action should be completed within 90 days from delivery of this Field Safety Notice.

4.	6. Anticipated timescale for follow-up FSN	Not planned yet.
4.	7. Manufacturer information (For contact details of local representative refer to page 1 of this FSN)	
	a. Company Name	Carnamedica Sp. z o.o.
	b. Address	21/U6 Olszynki Grochowskiej St.; 04-281 Warsaw; Poland
	c. Website address	www.carnamedica.com
4.	8. The Competent (Regulatory) Authority of your country has been informed about this communication to customers. *	
	YES	
4.	9. List of attachments/appendices:	<ul style="list-style-type: none"> • Appendix A – list of product references, lots and UDI codes • Appendix B – Instructions for the visual inspection • Distributor/Importer Reply Form • Customer Reply Form
4.	10. Name/Signature	Paweł Szczudło CEO
		Signature

	Transmission of this Field Safety Notice
	<p>This notice needs to be passed on all those who need to be aware within your organisation or to any organisation where the potentially affected devices have been transferred.</p> <p>Please maintain awareness on this notice and resulting action for an appropriate period to ensure effectiveness of the corrective action.</p> <p>Please report all device-related incidents to the manufacturer (vigilance@carnamedica.com), distributor or local representative, and the national Competent Authority if appropriate, as this provides important feedback.*</p>

Note: Fields indicated by * are considered necessary for all FSNs. Others are optional.

Appendix A – list of product references, batches and UDI codes



Reference number	LOT number	Product's name	UDI-DI code
BUWC	010722	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 010722 (17) 230707
BUWC	061022	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 061022 (17) 231210
BUWC	081222	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 081222 (17) 240212
BUWC	022422	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 022422 (17) 230824
BUWC	030222	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 030222 (17) 230902
BUWC	090122	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 090122 (17) 240301
BUWC	030322	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 030322 (17) 230903
BUWC	110922	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 110922 (17) 240509
BUWC	021822	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	(01) 5906874879221 (10) 021822 (17) 230818
BUWC	112122	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	N/A
BUWC	101822	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	N/A
BUWC	031122	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	N/A
BUWC	022822	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 1L	N/A
BUWC2000	030722	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879238 (10) 030722 (17) 230907
BUWC2000	010322	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879238 (10) 010322 (17) 230703
BUWC2000	030422	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879238 (10) 030422 (17) 230904
BUWC2000	030822	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879238 (10) 030822 (17) 230908
BUWC2000	123021	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879238 (10) 20211230 (17) 20230630
BUWC2000	030922	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879221 (10) 030922 (17) 230909
BUWC2000	030122	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	(01) 5906874879238 (10) 030122 (17) 230901
BUWC2000	082222	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	N/A
BUWC2000	082322	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	N/A
BUWC2000	061022	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	N/A
BUWC2000	022522	Belzer UW® Cold Storage Solutionl (University of Wisconsin Solution) 2L	N/A
BMPSC	110822	Belzer MPS® (UW Machine Perfusion Solution) 1L	(01) 5906874879245 (10) 110822 (17) 240508
BMPSC	121721	Belzer MPS® (UW Machine Perfusion Solution) 1L	(01) 5906874879245 (10) 20211217 (17) 20230617
BMPSC	121621	Belzer MPS® (UW Machine Perfusion Solution) 1L	(01) 5906874879245 (10) 20211216 (17) 20230616
SPRT	120822	StoreProtect® 1L	(01) 5906874879009 (10) 120822 (17) 240212

Appendix B – Visual inspection for the Health Care Professionals

We would appreciate your assistance in the following actions:

5. **Read** the “2.1. Description of the product problem” section of the attached FSN carefully to fully understand the issue involved.
6. Please immediately **examine** your inventory stock to determine if you have any remaining product in your possession (**see Appendix A to the FSN**).
7. **Stop** any further usage of the affected product.
8. The following illustrations are provided to help you identify the products and lots. Affected lots are identified by the reference number and lot number on the bag and case labels.

Bag labels

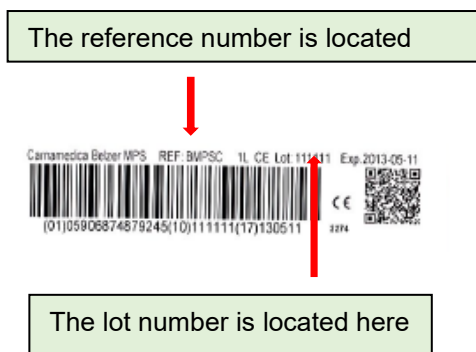


Container filled with organ perfusion and preservation solution
 Recipiente con la solución para perfusión y preservación de órganos
 Conteneur avec solution pour perfusion et conservation des organes
 Contenitore con soluzione per perfusione e conservazione degli organi
 Behälter mit Lösung zur Durchblutung und Konservierung der Organe
 Behållare med perfusionsvätska och vätskor för transplanterade organ
 Recipiente com a solução para preservação de órgãos
 Упаковка для перфузии и хранения органов, предназначенный для трансплантации
 330 mOsm/kg [Na] 101 mEq/L, [K] 25 mEq/L

Warning: Not intended for systemic administration by direct injection or intravenous infusion.	Warning: Not for in situ flushing of organs in living donors or patients.	Warning: Discard any unused portion.
Advertencia: No está destinado a la administración sistémica mediante inyección directa ni por perfusión intravenosa.	Advertencia: No apto para la irrigación de órganos in situ en donantes o pacientes vivos.	Advertencia: Deseché cualquier porción no utilizada.
Avertissement: Non destiné à une administration par voie générale et injection directe ou perfusion intraveineuse.	Avertissement: Non destiné au rinçage in situ d'organes sur les donneurs vivants ou les patients.	Avertissement: Jeter toute portion inutilisée.
Attenzione: Non destinato all'amministrazione sistemica mediante iniezione diretta o infusione endovenosa.	Attenzione: Non idoneo per il lavaggio in situ di organi in donatori o pazienti vivi.	Attenzione: Scartare eventuali residui.
Warnhinweis: Nicht zur systemischen Verabreichung durch Direktinjektion oder intravenöse Infusion bestimmt.	Warnhinweis: Nicht zur In-situ-Spülung von Organen im Körper lebender Spender oder Patienten.	Warnhinweis: Nicht verbrauchte Teil entsorgen.
Obavestiti: proizvod je namijenjen korištenju kao direktna injekcija ili infuzija.	Obavestiti: proizvod je predodređen korištenju kao organsko tkivo koje se koristi za transplantaciju.	Obavestiti: dio toga koji nije korišten treba odbaciti.
Aviso: Não se destina a administração sistémica por injeção direta ou infusão intravenosa.	Aviso: Não se destina à irrigação in situ de órgãos em doadores vivos ou doentes.	Aviso: Rejeitar qualquer porção não utilizada.
Внимание: не предназначен для инъекций и инфузий внутривенного назначения.	Внимание: не использовать для промывки органов живым донорам и пациентам.	Внимание: отбраковать часть продукта, которая была использована.

The reference number is located here

The lot number is located here



Case label



The lot number is located here

The reference number is located here

5. **Conduct** a physical count and **record** the data on the Customer Reply Form (in case of the hospitals/ clinics/ etc.) attached to the FSN.
6. **Perform** and additional visual inspections according to this Appendix to identify bags of solution that may represent leaking, discoloration, and contamination with particles prior to use of product.
Should you have any existing product from the lots above or identify any units of solution containing leakage, discoloration or signs of contamination take immediate action to quarantine and report this information.
Only fluid presenting a colourless appearance should be considered uncontaminated.
Before any use of the product, check their condition according to the IFU (Instructions for Use), section **PREPARATION**.

UNCONTAMINATED BAG	
<p>Description:</p> <p>The solution is a clear to slightly yellow, sterile. No leakages from the bag.</p> <p>The bag is properly labeled, clear and dry and free from moisture.</p>	

CONTAMINATED BAG

LEAKAGE

Description:
Picture of Leaking Bag



TURBIDITY/ DISCOLORATION

Description:
Picture of the turbid/
discolored solution





7. **Dispose** of the affected products through waste system, recycle packaging and **document** that on the Customer Reply Form attached to this Notice. If there is no possibility to dispose of the product in this way, you may return the product to local Customer representative through your normal means.
8. **Return** the Customer Reply Form to:
 - your local representative/ distributor (in country BTL representative: f.harvey@b2ll.com and m.harper@b2ll.com);
 - or via e-mail to vigilance@carnamedica.com.This is important to complete even, if you have no affected product on hand. Please ensure the form contains a contact name and signature.
9. **Contact** your local representative/ distributor (in country BTL representative or <https://bridgetolife.eu/contact-bridge-to-life-ltd/>) or Carnamedica's Customer Service on office@carnamedica.com to understand how to obtain a credit note against affected product.
10. **Maintain** awareness of this Notice until all affected product has been inspected/ destroyed.
11. **Share** this Notice with anyone who needs to be informed in your facility, or in any facility where potentially affected devices may have been transferred.
12. For any questions about this process, please **contact** your local representative/ distributor (in country BTL representative Mr. Mark Harper – Bridge to Life QA Director – m.harper@B2LL.com) or Carnamedica at vigilance@carnamedica.com.

